



[I-21/17/2025-W&M Section]

GOVERNMENT OF INDIA/भारत सरकार
MINISTRY OF CONSUMER AFFAIRS, FOOD AND PUBLIC DISTRIBUTION
उपभोक्ता मामले, खाद्य एवं सार्वजनिक वितरण मंत्रालय
DEPARTMENT OF CONSUMER AFFAIRS/ उपभोक्ता मामले विभाग
LEGAL METROLOGY DIVISION/ विधिक मापविज्ञान प्रभाग

Krishi Bhawan, New Delhi /कृषि भवन, नई दिल्ली
Dated/दिनांक:- 10.03.2025

Certificate of Approval of Model/ मॉडल का अनुमोदन प्रमाणपत्र


Whereas the Central Government, after considering the report submitted to it by prescribed authority, is satisfied that the model described in the said report (see the figure given below) is in conformity with the provisions of the Legal Metrology Act, 2009 (1 of 2010) and the Legal Metrology (Approval of Models) Rules, 2011 and the said model is likely to maintain its accuracy over periods of sustained use and to render accurate service under varied conditions;

Now, therefore, in exercise of the powers conferred by section 22 of the Legal Metrology Act, 2009 (1 of 2010) read with sub-rule (6) of rule 8 and sub-rule (4) of rule 11 of the Legal Metrology (Approval of Models) Rules, 2011, as per OIML R 51, the Central Government hereby issues the certificate of approval of the model of automatic catch weighing instrument (check weigher) belonging to accuracy class XIII(x), where $x=1$ of series "SSP-CW" and with brand name "BEW-DA" (hereafter in referred to as the said model), manufactured by M/s. BEW-DA ENGINEERS PRIVATE LIMITED 001, Aleen Park, Shriprastha, 2nd Road, Opp Mother Merry School, Nallasopara West cityname Palghar Maharashtra-401203 and which is assigned the approval mark IND/09/25/ 78 (the picture of the model is given below as Figure 1);


Technical Data:

Type of instrument	Automatic Catch Weighing Instrument(check weigher)
Procedure Adopted for testing & Conformity	OIML R 51
Working Principle	Strain gauge type load cell based
Accuracy class	XIII(x), where class designation factor $x=1$,
Maximum capacity	10 kg
Minimum capacity	1kg
Scale interval (e)	1 g
Belt Speed	45 packs per minute (max)
Belt Size/ Load Receptor	620mm × 500 mm
Detail of Load cell	Make: VPG Transducers Brand Name : Tedeia-Huntleigh Model: 1042 Accuracy Class: C6 Type: Bending beam load cell with strain gauge
Power Supply	230 V AC
Display	Touch screen Liquid Crystal Display (LCD)

Figure 1

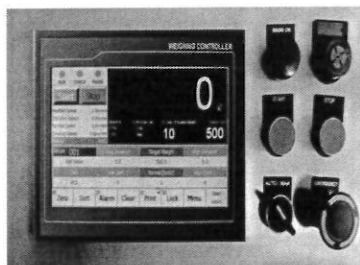

Max = 10 kg, e = 1 g, Min capacity = 1 kg, Class = XIII(x) where Class designation factor x=1,
Brand Name = BEW-DA, Model Series = SSP-CW series.

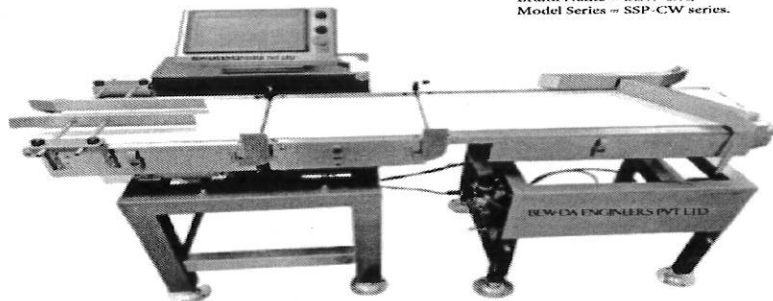

Max = 10 kg, e = 1 g,
Min capacity = 1 kg,
Class = XIII(x), Class designation factor x=1
Brand Name = BEW-DA,
Model Series = SSP-CW series.

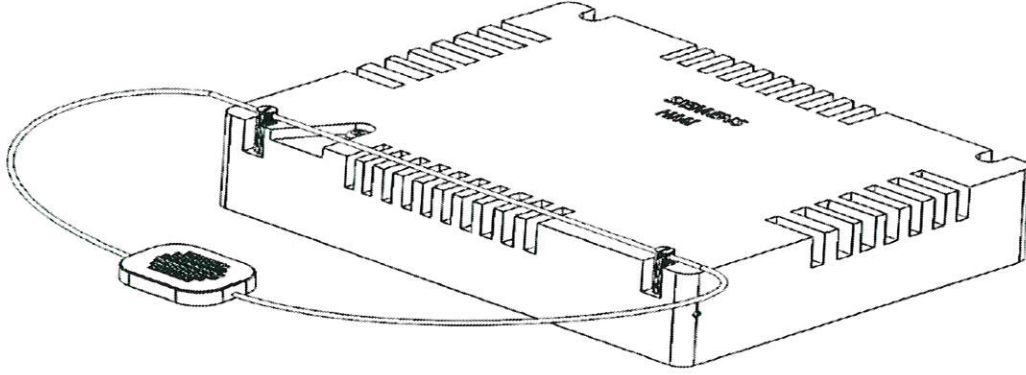


Figure 2

The box is sealed with wire and lead seal for calibration protection. A typical schematic diagram of sealing provision to prevent the fraudulent practices of the model is given above as Figure 2. A dip switch has also been provided in mother board/PCB to disable access to external calibration.

Further, in exercise of the power conferred by sub-rule (9) of rule 8 of the Legal Metrology (Approval of Models) Rules, 2011, the Central Government hereby declares that this certificate of approval of the said model shall also cover the Automatic Catch Weighing Instrument (check weigher) of similar make, accuracy and performance of same series with maximum capacity up to 25 kg with number of verification scale interval (n) in the range of 500 to 10000 for 'e' value of 5g or more and with number of verification scale interval (n) in the range of 100 to 10000 for 'e' value of 100mg to 2g with 'e' value of 1×10^k , 2×10^k or 5×10^k , where k is a positive or negative whole number or equal to zero manufactured by the same manufacturer in accordance with the same principle, design and with the same materials with which, the said approved model has been manufactured.

[F.No. I-21/17/2025-W&M Section]

आशुतोष अग्रवाल

Director (Legal Metrology) to Govt. of India/ निदेशक (विधिक माप विज्ञान) भारत सरकार

Phone/दूरभाष 01123389489

Email/ई-मेल: dirwm-ca@nic.in

Online Application No. 18880