



[I-21/112/2025-W&M Section]

GOVERNMENT OF INDIA/भारत सरकार
MINISTRY OF CONSUMER AFFAIRS, FOOD AND PUBLIC DISTRIBUTION
उपभोक्ता मामले, खाद्य एवं सार्वजनिक वितरण मंत्रालय
DEPARTMENT OF CONSUMER AFFAIRS/ उपभोक्ता मामले विभाग
LEGAL METROLOGY DIVISION/ विधिक मापविज्ञान प्रभाग

Krishi Bhawan/कृषि भवन, नई दिल्ली
Dated/दिनांक:- 07.05.2025

Certificate of Approval of Model/ मॉडल का अनुमोदन प्रमाणपत्र

Whereas the Central Government, after considering the report submitted to it by the prescribed authority, is satisfied that the model described in the said report is in conformity with the provisions of the Legal Metrology Act, 2009 (1 of 2010) and the Legal Metrology (Approval of Models) Rules, 2011 and the said model is likely to maintain its accuracy over periods of sustained use and to render accurate service under varied conditions;


Now, therefore, in exercise of the powers conferred by section 22 of the Legal Metrology Act, 2009 (1 of 2010) read with sub-rule (6) of rule 8 and sub-rule (4) of rule 11 of the Legal Metrology (Approval of Models) Rules, 2011, as per Schedule Eighth of the Legal Metrology (General) Rules, 2011, the Central Government hereby issues the certificate of Measuring systems for liquids other than water with digital indication of Accuracy Class 0.5 of series "Centralized Lube Management System-LUBINET" with brand name "ATS ELGI" (here in after referred to as the said model), manufactured by M/s. ATS ELGI LIMITED, Private Industrial Estate, Pollachi Main Road, SIDICO, Kurichy, Coimbatore-641021 and which is assigned the approval mark IND/09/25/155 (the picture of the model is given below as Figure 1);

The said model is used for inventory management and is not for retail sale.

Technical Data:

Accuracy class	0.5
Maximum Flow Rate	5 lpm
Minimum Flow Rate	2 lpm
Minimum Measured Quantity(MMQ)	1000 ml
Resolution/Smallest Division	10 ml
Non resettable Totalizer	12 digits
Volume Display	4 digits
Display Type	LCD and LED for individual nozzles
No.of Nozzles	8
Power Supply	230 V AC / 24 V DC
Intended use	To deliver the lubricating oil and similar products

Figure 1

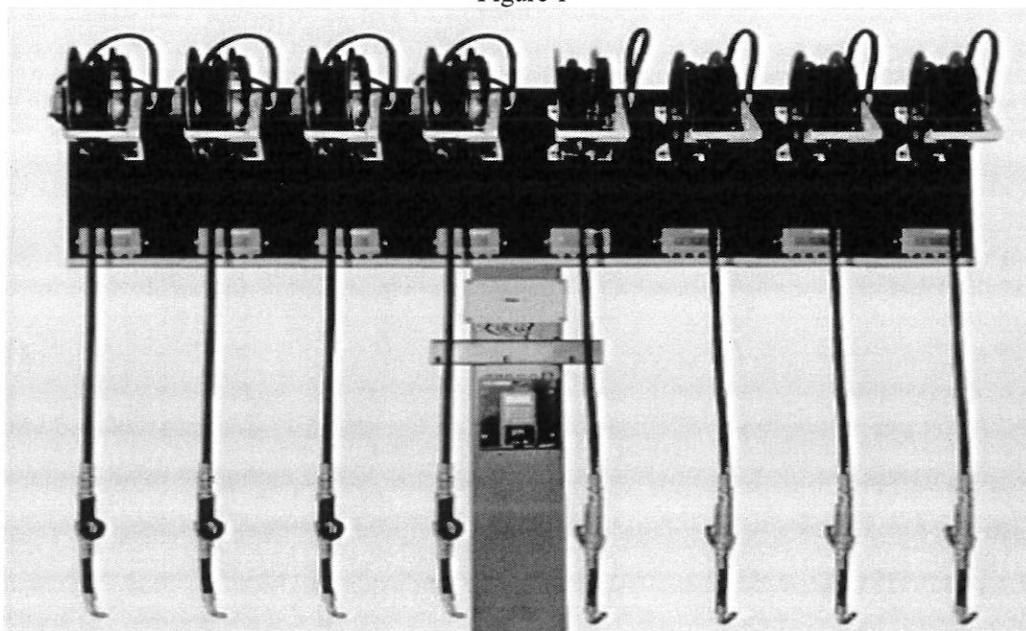

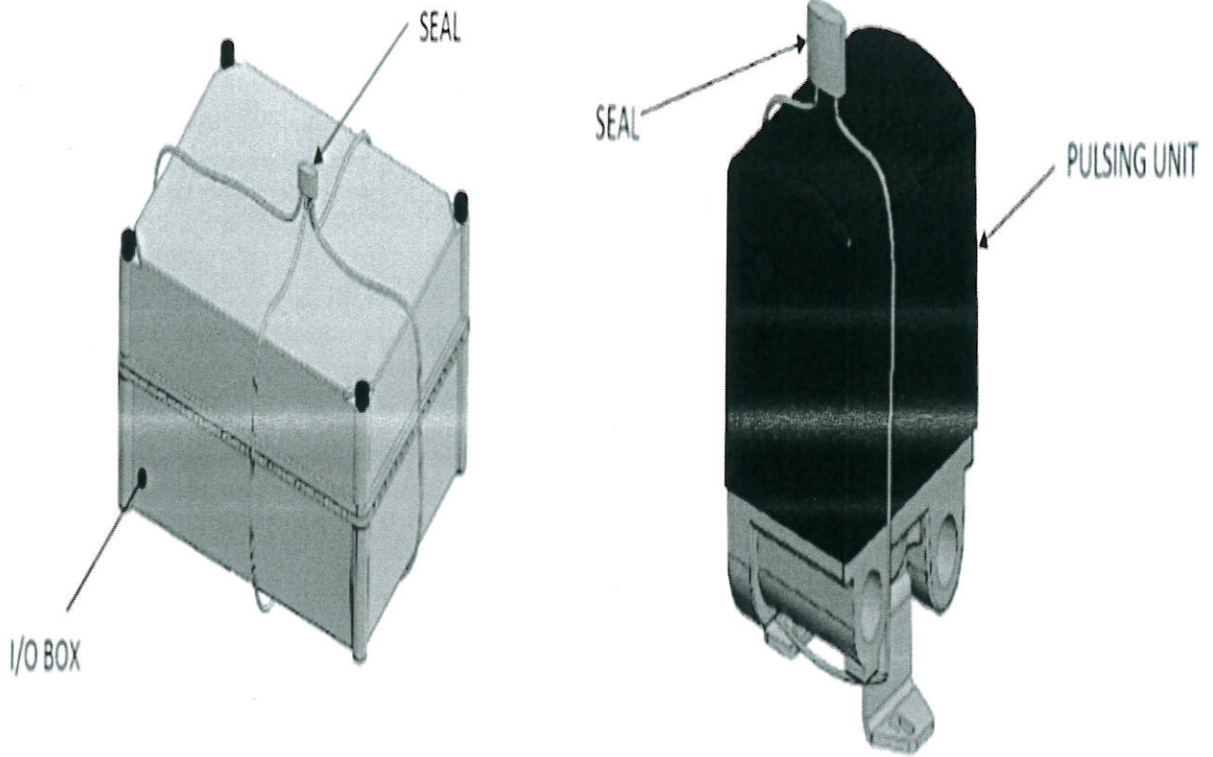


Figure 2.

A typical schematic diagram of sealing provision to prevent the fraudulent practices of the model is given above as Figure 2.

[F.No. I-21/112/2025-W&M]

Ashutosh Agarwal

(Ashutosh Agarwal) / (आशुतोष अग्रवाल)
Director (Legal Metrology)/निदेशक (विधिक माप विज्ञान)
Phone/दूरभाष: 01123389489
Email/ई-मेल: dirwm-ca@nic.in

Online Application: 22080