



[I-21/62/2025-W&M Section]

GOVERNMENT OF INDIA/भारत सरकार
MINISTRY OF CONSUMER AFFAIRS, FOOD AND PUBLIC DISTRIBUTION
उपभोक्ता मामले, खाद्य एवं सार्वजनिक वितरण मंत्रालय
DEPARTMENT OF CONSUMER AFFAIRS/ उपभोक्ता मामले विभाग
LEGAL METROLOGY DIVISION/ विधिक मापविज्ञान प्रभाग

Krishi Bhawan/कृषि भवन, नई दिल्ली

Dated/दिनांक:- 15.04.2025

Certificate of Approval of Model/ मॉडल का अनुमोदन प्रमाणपत्र

Whereas the Central Government, after considering the report submitted to it by the prescribed authority along with the OIML-CS certificate: R76/2006-A-NL1-21.2 issued by Netherland is satisfied that the model described in the said report (see the figure given below), is in conformity with the provisions of the Legal Metrology Act 2009(1 of 2010) and the Legal Metrology (Approval of Models) Rules, 2011 and the said model is likely to maintain its accuracy over periods of sustained use and to render accurate service under varied conditions;

Now, therefore, in exercise of the powers conferred by section 22 of the Legal Metrology Act, 2009 (1 of 2010) read with sub-rule (6) of rule 8 and sub-rule (4) of rule 11 of the Legal Metrology (Approval of Models) Rules, 2011, the Central Government hereby issues the certificate of approval of the model of Non automatic weighing instrument of Model: Q1 100" of accuracy class III, and with brand name "BIZERBA" (hereinafter referred to as the said model), manufactured by M/s Bizerba SE & Co. KG and imported & marketed in India without any alteration before or after sale by M/s BIZERBA INDIA Pvt. Ltd. , City Name PUNE Maharashtra - 411057 which is assigned the approval mark IND/09/25/123 (the picture of the model is given below as Figure 1);

Figure 1





Technical Data:

Accuracy class	III
Maximum capacity	$\text{Max} \leq 30 \text{ kg}$
Verification scale interval	$e \geq 1 \text{ g}$
Weighing range(s)	Single interval Multi-interval
Maximum number of scale intervals	$n \leq 6000$
Maximum number of scale intervals (multi-interval)	$n \geq 3000$ (per partial weighing range)
Maximum number of partial weighing ranges	2
Temperature range	$-10^\circ\text{C} / +40^\circ\text{C}$
Power supply voltage	120 – 240 V AC 50/60 Hz
Application	Intended to be used for direct sales to the public

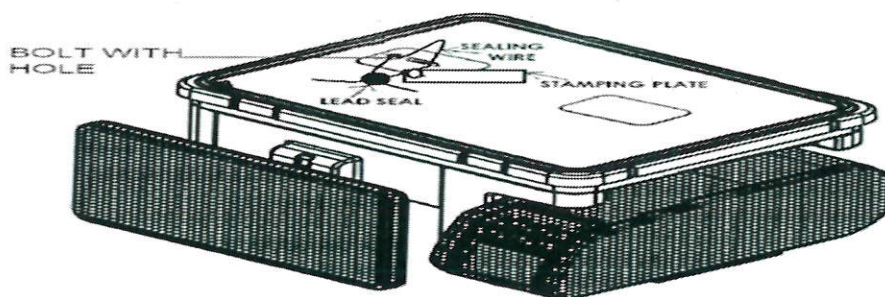


Figure-2

Sealing is done in the device by passing sealing wire through holes in the two sealing nuts fitted on the back of the device. The seal wire is passed through the holes of the sealing nuts and fastened by a lead seal for verification stamp. A typical Schematic Diagram of sealing provision of the said model is given as above. This instrument has an external calibration facility through a switch provided on Housing to disable the access to external calibration control. This is not accessible for calibration without breaking/tampering with this seal.

[F.No.I-21/62/2025-W&M Section]

(Signature)

(Ashutosh Agarwal/आशुतोष अग्रवाल)
Director (Legal Metrology) to Govt. of India/ निदेशक (विधिक माप विज्ञान) भारत सरकार
Phone/दूरभाष 01123389489
Email/ई-मेल: dirwm-ca@nic.in

Online application no. 19884