



Online Application No. 23792

[I-21/131/2026-W&M Section]
GOVERNMENT OF INDIA/भारत सरकार
MINISTRY OF CONSUMER AFFAIRS, FOOD AND PUBLIC DISTRIBUTION
उपभोक्ता मामले, खाद्य एवं सार्वजनिक वितरण मंत्रालय
DEPARTMENT OF CONSUMER AFFAIRS/ उपभोक्ता मामले विभाग
LEGAL METROLOGY DIVISION/ विधिक मापविज्ञान प्रभाग

Krishi Bhawan/कृषि भवन, नई दिल्ली
Dated/दिनांक:- 13.5.2026

Certificate of Approval of Model/ मॉडल का अनुमोदन प्रमाणपत्र

Whereas the Central Government, after considering the report submitted to it by prescribed authority, is satisfied that the model described in the said report (see the figure given below) is in conformity with the provisions of the Legal Metrology Act, 2009 (1 of 2010) and the Legal Metrology (Approval of Models) Rules, 2011 and the said model is likely to maintain its accuracy over periods of sustained use and to render accurate service under varied conditions;

Now, therefore, in exercise of the powers conferred by section 22 of the Legal Metrology Act, 2009 (1 of 2010) read with sub-rule (6) of rule 8 and sub-rule (4) of rule 11 of the Legal Metrology (Approval of Models) Rules, 2011, as per OIML R 49, the Central Government hereby issues the certificate of approval of the model of water meter (Ultrasonic) of accuracy class 2 (hereinafter referred to as the said model) of series "VIFLOW-UFM-013" and with brand name "VISION WORLDTECH" manufactured by M/s Vision World Tech Private Limited, A-15, Jai Ambey Nagar, Infront of Jaipur Hospital , Tonk Road,Jaipur,Rajasthan-302018 and which is assigned the approval mark IND/09/26/ 219 (the picture of the model is given below as Figure 1);

The said model is a water meter (ultrasonic) which is based on principle of ultrasonic sensing.

Technical Data:

Accuracy Class	2
Tested as per standard	OIML R 49
DN Size	50 mm
Verification scale interval	0.001m ³
Flow Rates	Q ₁ = 0.40 m ³ /h Q ₂ = 0.64 m ³ /h Q ₃ = 40 m ³ /h Q ₄ = 50 m ³ /h
Type of Display	LCD
No.of digits	9 (999999.999 m ³)
Power Supply	3.6V DC
Software version	V1.2.2
Checksum	80a9776341a023b44c3da7cafa5d4407aab3dd872a21512915e419 64c5fcb408



Figure-1

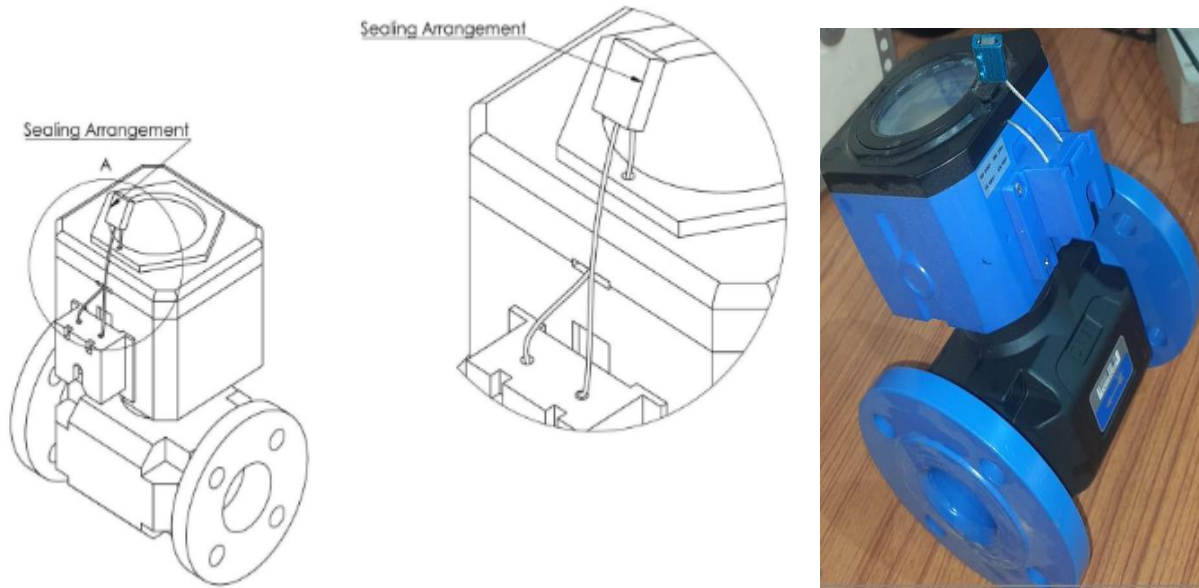


Figure 2

Sealing is done at two opposite points as indicated by the sealing arrangement. The calibration could not be performed/alterd without removing the seal and the top cover which acts as DIP switch. A typical schematic diagram and photograph of sealing provision to prevent the fraudulent practices of the model is given above as Figure 2.

[F.No. I-21/131/2026-W&M Section]



(Ashutosh Agarwal/आशुतोष अग्रवाल)
Director (Legal Metrology) to Govt. of India/ निदेशक (विधिक माप विज्ञान) भारत सरकार
Phone/दूरभाष -01123389489
Email/ई-मेल: dirwm-ca@nic.in