Revised

Online Application: 25285

[I-21/232/2026-W&M Section]

GOVERNMENT OF INDIA/भारत सरकार

MINISTRY OF CONSUMER AFFAIRS, FOOD AND PUBLIC DISTRIBUTION

उपभोक्ता मामले, खाद्य एवं सार्वजनिक वितरण मंत्रालय

DEPARTMENT OF CONSUMER AFFAIRS/ उपभोक्ता मामले विभाग

LEGAL METROLOGY DIVISION/ विधिक मापविज्ञान प्रभाग

Krishi Bhawan/कृषि भवन, नई दिल्ली

Dated/दिनांक:- 04 .11.2026

Certificate of Approval of Model/ मॉडल का अनुमोदन प्रमाणपत्र

Whereas the Central Government, after considering the report submitted to it by the prescribed authority along with the OIML-CS certificate: R76/2006-A-NL 1-23.04 revision 1 issued by NMi Netherlands is satisfied that the model described in the said report (see the figure given below), is in conformity with the provisions of the Legal Metrology Act 2009 (1 of 2010) and the Legal Metrology (Approval of Models) Rules, 2011 and the said model is likely to maintain its accuracy over periods of sustained use and to render accurate service under varied conditions;


Now, therefore, in exercise of the powers conferred by section 22 of the Legal Metrology Act, 2009 (1 of 2010) read with sub-rule (6) of rule 8 and sub-rule (4) of rule 11 of the Legal Metrology (Approval of Models) Rules, 2011, the Central Government hereby issues the certificate of approval of the model of Non Automatic Weighing Instrument of Type: "MP72X1 single interval", "MP72X2 multi-interval" , "MP72X3 single-interval with calibration push button" , "MP72X4 multi-interval with calibration push button" where 'X' denotes alternative variants not affecting metrological parameters and with brand name "Zebra" (hereinafter referred to as the said model), manufactured by Zebra Technologies Corp 1 Zebra Plaza, Holtsville, NY 11742, United State of America and imported & marketed in India without any alteration before or after sale by M/s Markss Infotech Limited 70B, Kandivali Indl. Estate, M.G. Road, Charkop kandivali, Mumbai Suburban, Maharashtra, 400067 which is assigned the approval mark IND/09/26/ 490 (the picture of the model is given below as Figure 1).

Figure 1



Technical Data:

Accuracy Class	III
Maximum capacity	Max ≤ 15 kg
Verification scale interval	e ≥ 2 g
Weighing ranges	Single interval Multi-interval
Maximum number of scale intervals (one weighing range)	n ≤ 3000
Maximum number of scale intervals (multi-interval)	n ≤ 3000 (per partial weighing range)
Maximum number of partial weighing ranges	2
Temperature range	0 °C / +40 °C
Power supply voltage	100 – 240 V AC 50/60 Hz 12 V DC
Software identification Version number	1.04F

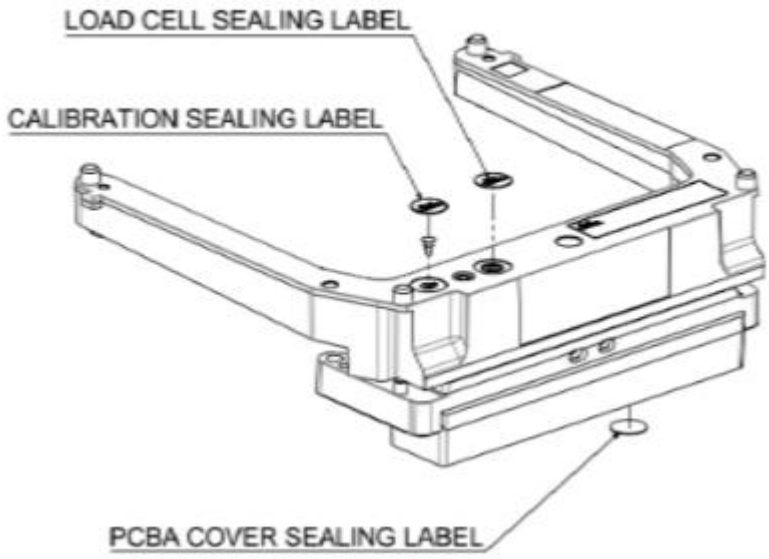

A typical schematic diagram of sealing provision to prevent the fraudulent practice of the model is given above as Figure (2).

[F.No.I-21/232/2026-W&M Section]

ASHUTOSH AGARWAL
Digitally signed by ASHUTOSH AGARWAL
Date: 2026.11.04 14:16:24 +05'30'

(Ashutosh Agarwal/आशुतोष अग्रवाल)
Director (Legal Metrology) to Govt. of India/ निदेशक (विधिक माप विज्ञान) भारत सरकार
Phone/दूरभाष 01123389489
Email/ई-मेल: dirwm-ca@nic.in